



S1P (Human) ELISA Kit

Catalog Number KA6338

96 assays

Version: 01

Intended for research use only

Table of Contents

Introduction	3
Intended Use.....	3
Background	3
Principle of the Assay	3
General Information	4
Materials Supplied.....	4
Materials Required but Not Supplied	4
Storage Instruction	4
Precautions for Use	4
Assay Protocol	5
Reagent Preparation.....	5
Sample Preparation	5
Assay Procedure	6
Data Analysis.....	8
Calculation of Results.....	8
Performance Characteristics	9
Resources.....	10
Plate Layout	10

Introduction

Intended Use

S1P (Human) ELISA kit is based on the Competitive ELISA principle to quantitatively measure the concentration of Sphingosine-1-phosphate in human serum, plasma, and other biological fluids.

Background

Sphingosine-1-phosphate (S1P) is a bioactive sphingolipid metabolite that is generated by the phosphorylation of sphingosine by sphingosine kinase 1 or 2. It is present in low concentrations in tissues such as lymphoid organs and thymus but is present in high concentrations in the blood, usually bound to ApoM in HDL particles. It acts as an intracellular second messenger as well as an extracellular ligand for G-protein-coupled receptors. S1P is implicated in a large number of physiological and cellular processes such as cell survival, immune cell trafficking, apoptosis, atherosclerosis, inflammation, angiogenesis, and tumorigenesis. Thus S1P could serve as a promising target for the treatment of human diseases.

Principle of the Assay

Test samples, Standards, and Biotinylated Detection antibody are added to the wells pre-coated with capture antibody and then washed with Wash Buffer. The HRP-Streptavidin is added and any unattached conjugates are washed off using Wash Buffer. The HRP enzymatic reaction is detected by the addition of TMB-substrate. Finally, the reaction is terminated with an acidic stop solution. The color developed is inversely proportional to the concentration of S1P in the sample or standard.

General Information

Materials Supplied

List of component

Component	Amount	Storage temp.
Micro ELISA Plate	8 x 12 well strips	-20°C
Standard (Lyophilized) (200ng)	2 vials	
Sample/Standard Dilution Buffer	20 mL	4°C
Biotin-labeled Antibody	60 µL	4°C (Avoid Light)
Antibody Dilution Buffer	10 mL	4°C
HRP-Streptavidin Conjugate (SABC)	120 µL	4°C (Avoid Light)
SABC Dilution Buffer	10 mL	4°C
TMB Substrate Solution	10 mL	4°C (Avoid Light)
Stop Solution	10 mL	4°C
Wash Buffer (25x)	30 mL	4°C
Plate Sealers	5 slides	4°C

Materials Required but Not Supplied

- Microplate reader capable of measuring absorbance at 450 nm
- 37°C incubator
- Precision pipettes with disposable tips
- Distilled or deionized water
- Clean eppendorf tubes for preparing standards or sample dilutions
- Absorbent paper

Storage Instruction

An unopened kit can be stored at 4°C for up to 6 months. If the kit is not used within 1 month, store the items separately according to the above-mentioned conditions once the kit is received.

Precautions for Use

FOR RESEARCH USE ONLY! Not to be used on humans.

Assay Protocol

Reagent Preparation

Note: Prepare reagents within 30 minutes before the experiment. Before using the kit, spin tubes and bring down all components to the bottom of tubes

- ✓ **Biotin-labeled Antibody working solution:** Prepare this working stock 1 hour prior to the start of the experiment. Calculate the total volume of the working solution: 0.05 mL/well x quantity of wells. Add 0.1 – 0.2 mL to the total volume. Dilute the Biotin-labeled antibody with Antibody Dilution Buffer at 1:100. Mix thoroughly.
- ✓ **HRP-Streptavidin Conjugate (SABC):** Prepare this working stock 30 minutes prior to the start of the experiment. Calculate the total volume of the working solution: 0.1 mL/well x quantity of wells. Add 0.1 – 0.2 mL to the total volume. Dilute the SABC with SABC Dilution Buffer at 1:100. Mix thoroughly.
- ✓ **Wash Buffer:** Dilute 25X Wash Buffer to 1X by adding 30 mL of 25X Wash Buffer and make up the volume to 750 mL with deionized/distilled water. If crystals present in the 25X Wash Buffer, warm it in water bath at 40°C. Mix it gently. The solution must be cooled to room temperature before use.
- ✓ **Standard Preparation:**
 - Add 1 mL Sample Dilution Buffer into one Standard tube (labeled as zero tube). Keep the tube at room temperature for 10 minutes. Mix thoroughly.
 - Label 7 tubes with 1/2, 1/4, 1/8, 1/16, 1/32, 1/64 and blank respectively. Add 0.3 mL of the Sample Dilution Buffer into each tube. Add 0.3 mL of the above Standard solution (from zero tube) into 1st tube and mix them thoroughly.
 - Transfer 0.3 mL from 1st tube to 2nd tube and mix them thoroughly. Transfer 0.3 mL from 2nd tube to 3rd tube and mix them thoroughly, and so on. Sample Dilution Buffer was used for the blank control. (Note: Please use Standard Solutions within 2 hours of preparation).

Sample Preparation

Note: Isolate the test samples soon after collecting, then, analyze immediately (within 2 hours). Or aliquot and store at -20°C (≤ 1 month) or -80°C (≤ 2 months). Avoid multiple freeze-thaw cycles. The hemolytic samples are not suitable for this assay.

- Serum: Place whole blood sample at room temperature for 2 hours or put it at 2 - 8°C overnight and centrifugation for 20 minutes at approximately 1000xg, Collect the supernatant and carry out the assay immediately. Blood collection tubes should be disposable, non-pyrogenic, and endotoxin free.
- Plasma: Collect plasma using EDTA-Na₂ or heparin as an anticoagulant. Centrifuge samples for 15 minutes at 1000xg at 2 -8°C within 30 minutes of collection. Collect the supernatant and carry out the assay immediately. Avoid hemolysis, high cholesterol samples.
- Tissue homogenates: As hemolytic blood may affect the assay result, it is necessary to remove residual blood by washing tissue with pre-cooling PBS buffer (0.01 M, pH 7.4). Mince tissue after

weighing it and homogenize it in PBS (the volume depends on the weight of the tissue. Normally, 9 mL PBS would be appropriate to 1 gram tissue pieces. Some protease inhibitors are recommended to add into the PBS) with a glass homogenizer on ice. To further break the cells, you can sonicate the suspension with an ultrasonic cell disrupter or subject it to freeze-thaw cycles. The homogenates are then centrifuged for 5 minutes at 5000xg to get the supernatant. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3 mg.

- Cell culture supernatant: Centrifuge supernatant for 20 minutes at 1000xg at 2 - 8°C to remove insoluble impurity and cell debris. Collect the clear supernatant and carry out the assay immediately.
- Cell Culture Lysate: Commercial RIPA kits are recommended to follow the instructions provided. Generally, 0.5 mL RIPA lysis buffer would be appropriate to 2×10^6 cells, DNA must be removed. The total protein concentration was determined by BCA kit and the total protein concentration of each pore sample should not exceed 0.3 mg.
- Other biological fluids: Centrifuge samples for 20 minutes at 1000xg at 4°C. Collect the supernatant and carry out the assay immediately.

Note: End user should estimate the concentration of the target protein in the test sample first, and select a proper dilution factor to make the diluted target protein concentration fall in the optimal detection range of the kit.

Assay Procedure

Note: Bring all reagents and samples to room temperature 30 minutes prior to the assay. It is recommended that all standards and samples be run at least in duplicate. A standard curve should be run for each assay.

1. Prepare all reagents, samples and standards as instructed.
2. Wash plate 2 times with 1X Wash Buffer before adding standard, blank, sample and control wells.
3. Add 50 μ L of each standards or samples into appropriate wells. The blank well will contain only Sample/Standard Dilution Buffer.
4. Immediately add 50 μ L of Biotin-labeled Antibody working solution. Cover the plate with plate sealer. Gently tap to ensure mixing. Incubate at 37°C for 45 minutes.
5. Remove the cover and discard the plate content. Wash the plate 3 times with 1X Wash Buffer without letting the wells completely dry. Let it soak for 1-2 minutes, and then remove all residual wash-liquid from the wells by aspiration. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Tap the plate on absorbent filter papers or other absorbent materials.
6. Add 100 μ L of SABC working solution into each well, cover the plate and incubate at 37°C for 30 minutes.
7. Discard the solution and wash 5 times with 1X Wash Buffer as step 5.
8. Add 90 μ L of TMB substrate into each well, cover the plate and incubate at 37 °C in dark within 10-20 minutes. (Note: The reaction time can be shortened or extended according to the actual color change,

but not more than 30 minutes. The reaction can be terminated when apparent gradient appeared in standard wells).

9. Add 50 μ L of Stop Solution to each well. Read result at 450 nm within 20 minutes.

Data Analysis

Calculation of Results

For calculation, (the relative O.D.450) = (the O.D.450 of each well) – (the O.D.450 of Zero well). The standard curve can be plotted as the relative O.D.450 of each standard solution (Y) vs. the respective concentration of the standard solution (X). The target concentration of the samples can be interpolated from the standard curve. If the samples measured were diluted, multiply the dilution factor to the concentrations from interpolation to obtain the concentration before dilution.

✓ Typical Standard Curve

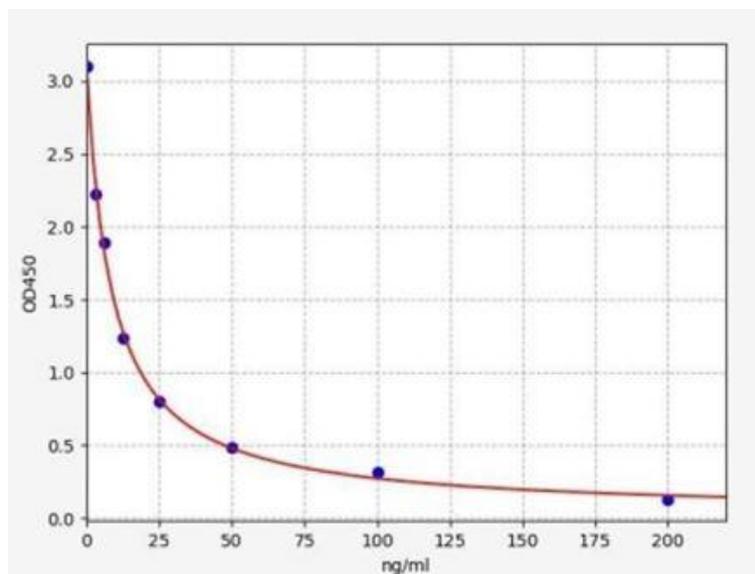


Figure: Typical Standard Curve and OD values: These standard curves are for demonstration only. A standard curve must be run with each assay.

STD. (ng/mL)	OD-1	OD-2	Average
0	3.058	3.146	3.102
3.125	2.193	2.257	2.225
6.25	1.869	1.923	1.896
12.5	1.216	1.252	1.234
25	0.794	0.818	0.806
50	0.48	0.494	0.487
100	0.309	0.317	0.313
200	0.128	0.132	0.13

Performance Characteristics

- ✓ Detection range: 3.125 - 200 ng/mL
- ✓ Sensitivity: 1.875 ng/mL
- ✓ Assay Precision: Intra-Assay CV < 8% and Inter-Assay CV < 10%
- ✓ Recovery range: 85 - 105% for normal human serum and plasma samples

Matrices mentioned below were spiked with certain level of Sphingosine-1-Phosphate and the recovery rates were calculated by comparing the measured value to the expected amount of Sphingosine-1-Phosphate in samples

Matrix	Recovery Range (%)	Average(%)
Serum (n=5)	89-105	99
EDTA Plasma (n=5)	85-102	97
Heparin Plasma (n=5)	87-98	94

- ✓ Linearity

Linearity of the assay kit was determined by spiking samples and their serial dilutions with appropriate concentration of Sphingosine-1-Phosphate. The results are represented as percentage of calculated concentration to the expected value.

Sample	1:2	1:4	1:8
Serum (n=5)	85-102%	87-103%	88-105%
EDTA Plasma (n=5)	83-101%	83-100%	85-95%
Heparin Plasma (n=5)	82-100%	85-99%	81-100%

This Competitive ELISA is highly sensitive and highly specific for the detection of Sphingosine-1-Phosphate in human samples. There is no significant cross-reactivity or interference between Sphingosine-1-Phosphate and analogues

Resources

Plate Layout

12								
11								
10								
9								
8								
7								
6								
5								
4								
3								
2								
1								
	A	B	C	D	E	F	G	H